


# Certificate

**Polymer Technology Systems Inc (PTS Diagnostics)**

using

**A1CNow+**

participated in the IFCC HbA1c Certification Programme to demonstrate traceability to the IFCC Reference Measurement Procedure and performed as shown below.

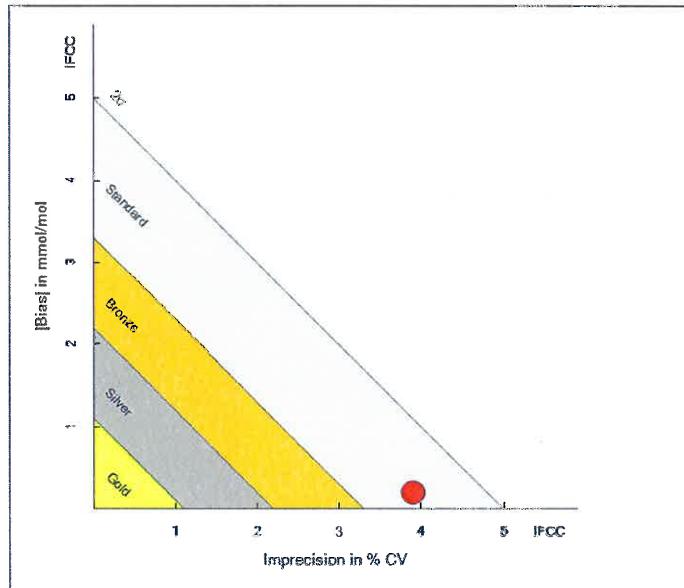


|               |          |          |
|---------------|----------|----------|
| Total Error = | 4.1      | mmol/mol |
| Bias =        | -0.2     | mmol/mol |
| Imprecision = | 3.9      | %        |
| Grade =       | Standard |          |

Criteria derived from the IFCC model for Quality Targets HbA1c (Clin Chem 2015;61 : 752-59)

Date of Certification : 01 January 2019

Date of Expiry : 01 January 2020



IFCC Network Coordinator  
Dr. C.W. Weykamp